

Combur¹⁰ Test[®] parameters

How to do it

- Collect urine sample in clean, sterile specimen container (preferably a disposable cup).
- Dip test strip into urine for not more than 1 second.
- When withdrawing the strip wipe side edge of the test strip along the rim of vessel to remove excess urine.
- After 60 seconds (leukocytes 60 – 120 seconds), compare reaction colours of the test patches with the colour scales on the label.
- Colour changes appearing only at the edges of the test patch or developing after more than 2 minutes are not relevant for diagnosis.


Some «do's» of urinalysis

- Use only clean, sterile urine specimen containers. Preferably disposable cups.
- Examination of the urine with test strips should be carried out as soon as possible, but within 2 hours at the latest. Mix the sample first.
- Always store the sample in the fridge (+4° C) if the urine test cannot be performed within 2 hours.
- The sample must be at room temperature for the test. Mix it first.
- Close the tube again immediately after removing the test strip.
- Store the test strips at a temperature between +2° and 30° C.
- Don't forget to write the patient's name on the urine specimen cup.

Some «don't's» of urinalysis

- Cleaning agents and disinfectants can distort results (false positive findings for blood and glucose).
- Freezing or centrifuging the urine destroys leucocytes and erythrocytes and renders the sample useless for further microscopic examination.
- If the urine is allowed to stand at room temperature for more than 2 hours, the composition changes (greatly increased bacterial growth). Never place the sample in direct sunlight.

Ascorbic acid – no problem with the Combur-Test[®] Product Line

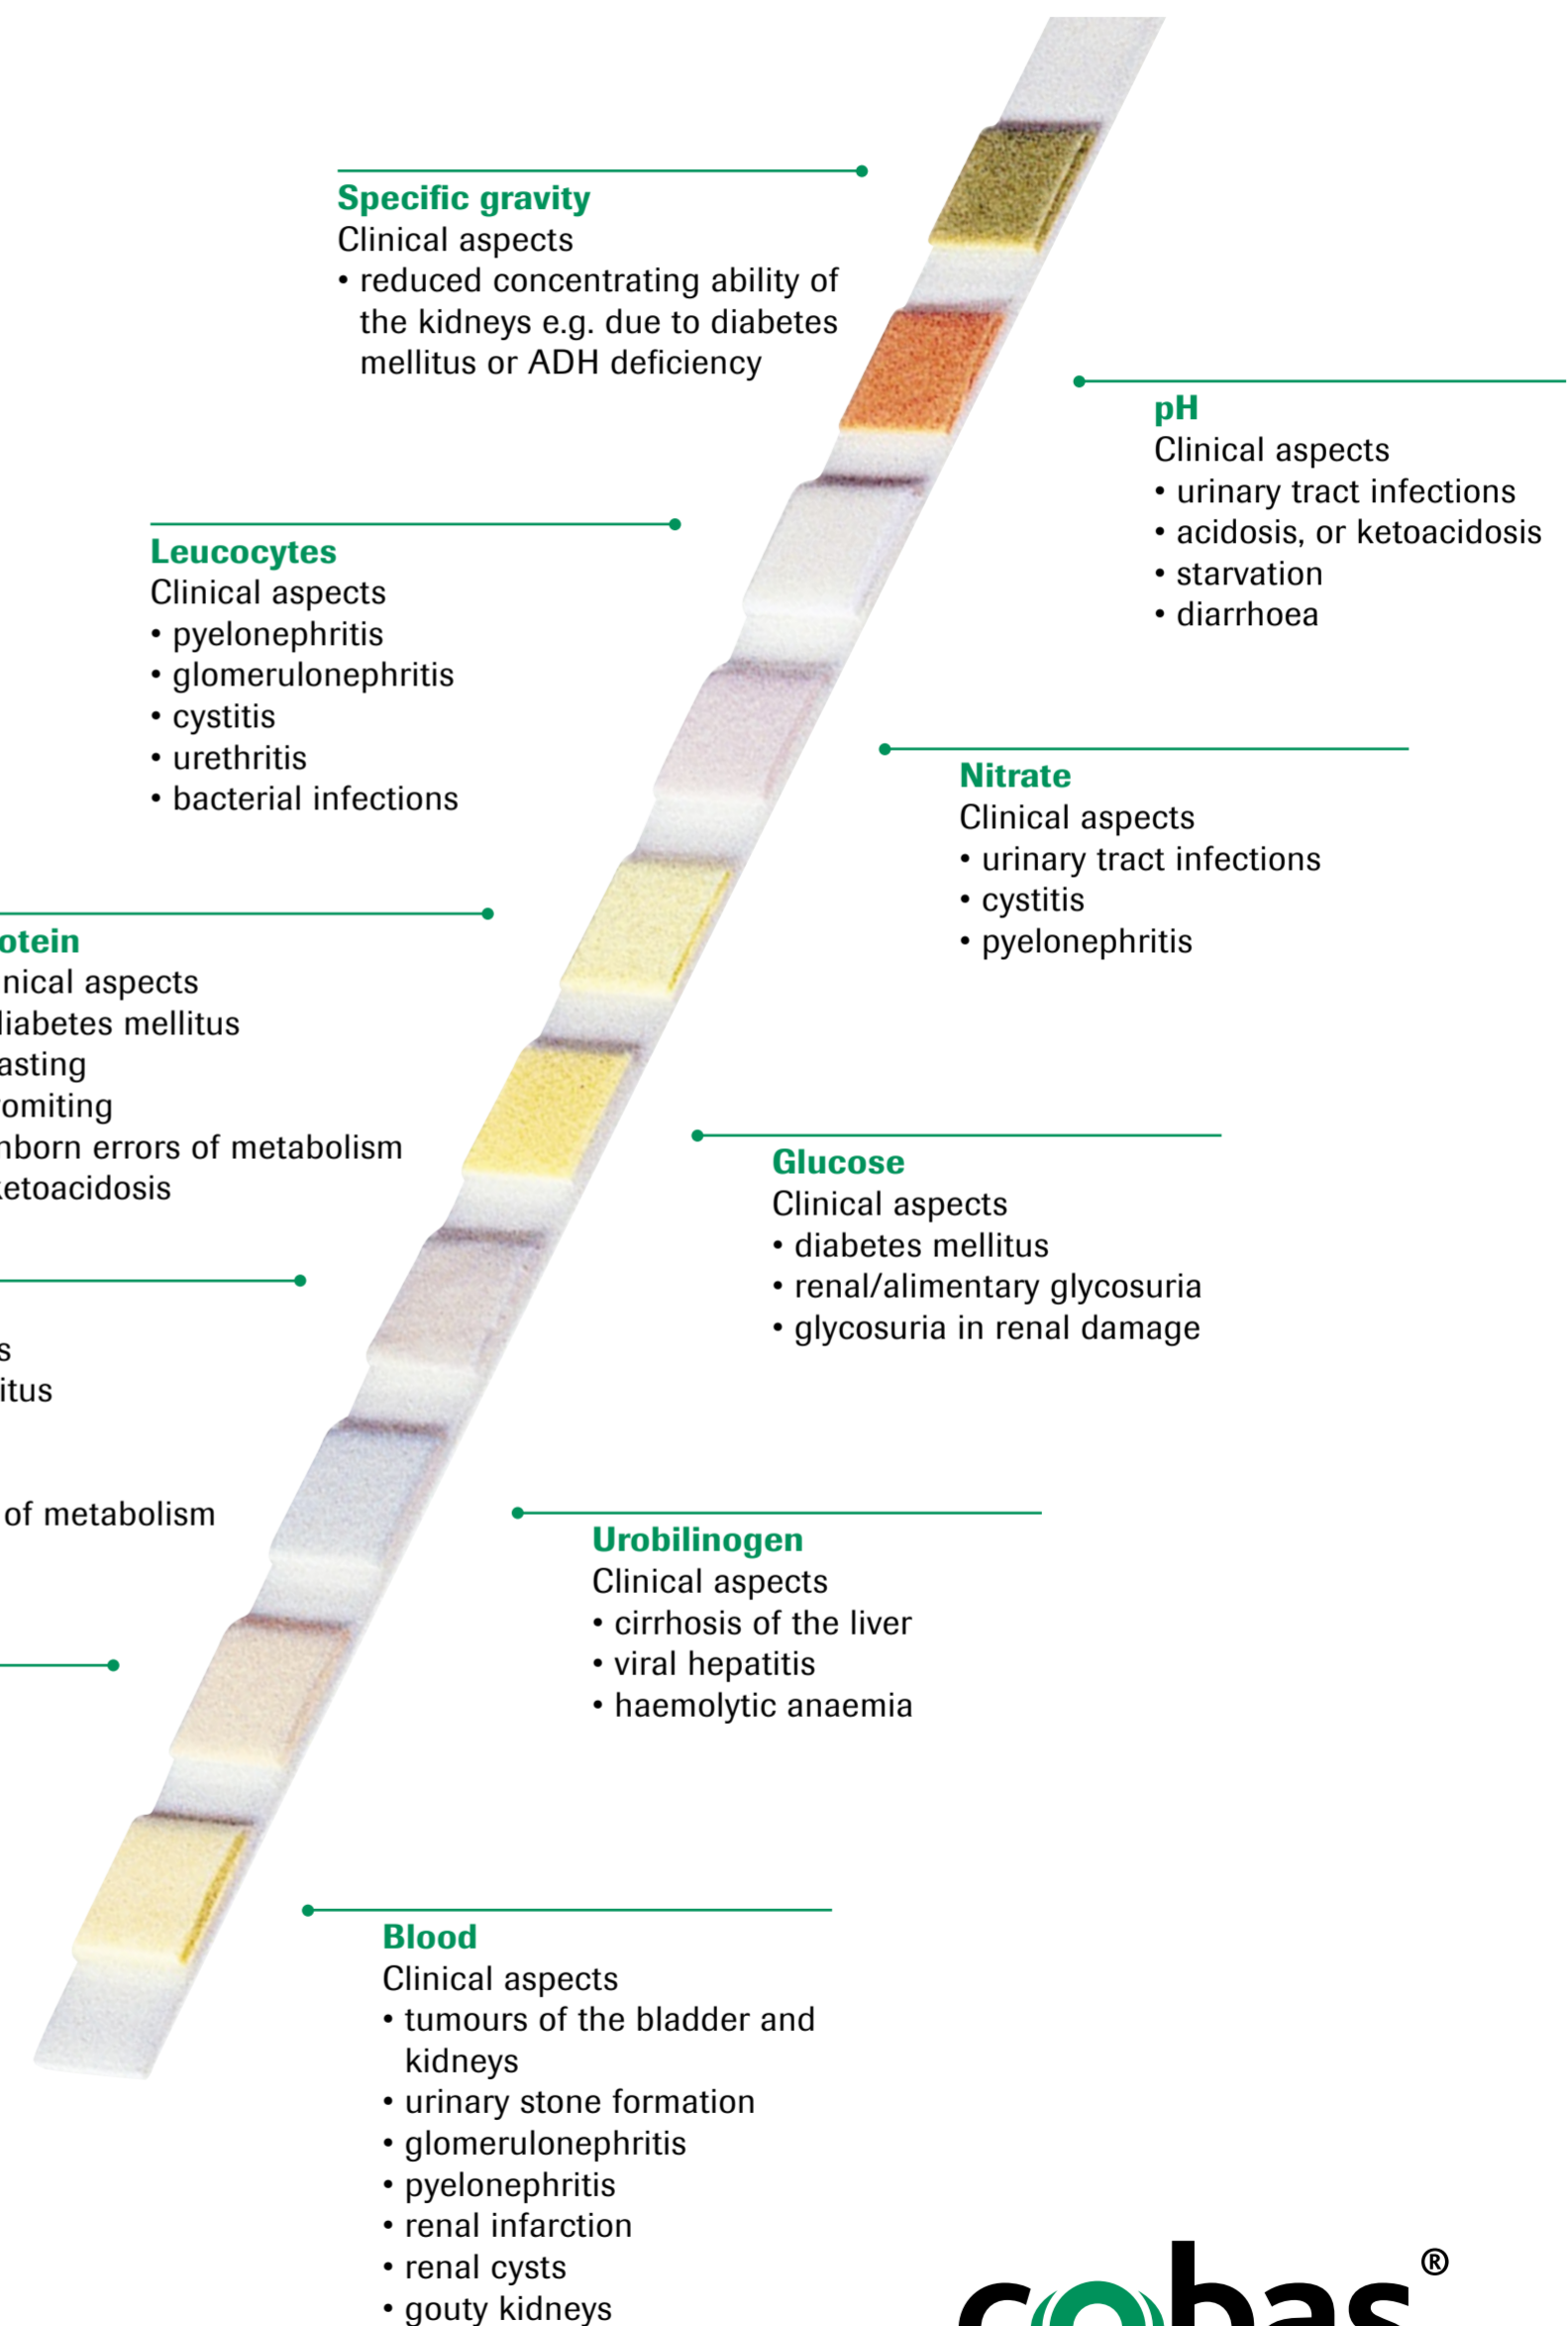

COBAS, COMBUR-TEST and LIFE NEEDS ANSWERS are trademarks of Roche.
© 2010 Roche
Roche Diagnostics Ltd. · CH-6343 Rotkreuz · Switzerland · www.roche.com

cobas[®]
Life needs answers